Chromatography





INTERNATIONAL

CARLO ERBA Reagents S.A.S

Chaussée du Vexin 27106 Val de Reuil To contact customer service : export@cer.dgroup.it

Ph.: +33 2 32 09 20 00 Fax: +33 2 32 09 20 20

- Chemicals for laboratory and industry: CARLO ERBA Reagents, an international recognized supplier of chemicals since 170 years, is specialised in high quality products, meeting your highest requirements: alcohols, solvents, minerals, buffers, acids in different grades, all included in a range of around 6000 references.
- Our two production facilities in France offer quality and service thanks to the flexibility and diversity of our production tools.
- A 8 500 m² international logistics platform ensure a level of service that meets your requirements.



- Our quality department, independent of our production, manages documentation, record controls, traceability, internal audits, change control, periodic monitoring of indicators, and continuous improvement.
- Certified ISO 9001: 2015 and ANSM inspection certificate for our 2 production sites.
- Global offer: 2 catalogues for a better service.... Chemicals et Labware









CARLO ERBA Reagents Your partner in choice



CARLO ERBA Reagents, a recognized chemical supplier for more than 170 years, operates at an international level in Analytical and Industrial Chemistry in the laboratory and industry sectors.


With its two production units, the CARLO ERBA Reagents Group offers its customers quality and service through the flexibility of production and installations Mixers up to 7000l, distillation columns, storage tanks, automated packaging lines, clean rooms are some of the technologies engineered to meet the vast range of the market needs.

Standard operational procedures for highly qualified operators for better plant management, permanent controls of all phases of production and packaging are the criteria that guide CARLO ERBA Reagents in its industrial activity.





In this brochure dedicated to chromatography, find in the first part a selection of chemicals (solvents, reagents, standards) specifically developed by CARLO ERBA Reagents for different types of chromatography.



- Solvents for UHPLC-MS
- Solvents, additives and blends for LC-MS
- Solvents for HPLC Gradient
- Solvents for HPLC Isocratic
- Solvents for HPLC preparative
- Mobile phases
- Silica gel and filter aids

Gas chromatography

- HEADSPACE solvents
- ATRASOL® solvents for the detection of traces in organic compounds and hydrocarbons
- ATRASOL® solvents for Hydrocarbon index determination according to ENISO9377-2
- GC-MS Solvents
- PESTIPUR® Solvents for pesticides residue analysis
- Organic standards

Ion Pair chromatography

Ionic chromatography

- Concentrated mobile phases
- Standard solutions

LIQUID CHROMATOGRAPHY

Leader in the market for solvents for chromatography and trace analysis, CARLO ERBA Reagents extended its range of solvents for HPLC in order to satisfy the ever increasing requirements in terms of equipment and detection methods. A particular emphasis was placed on impurities which, by interaction, can affect the result's reliability.

Our solvents for HPLC meet the requirements for this analytical technique by guaranteeing the optimal specifications on the following elements:

- Purity
- Non volatile residue content
- UV Transmission

ANALYSIS METHOD

	HPLC Preparative	HPLC Isocratic mode	HPLC Gradient mode	LC-MS	UHPLC	UHPLC-MS
RS HPLC Preparative						
RS HPLC Isocratic						
RS HPLC PLUS Gradient						
RS HPLC GOLD Ultra Gradient						
RS HPLC-MS						
RS UHPLC-MS						

In this easy-to-consult document, we offer you a choice of products specifically adapted for the preparation and analysis of your HPLC samples:

CARLO ERBA Reagents GRADES

- Solvents for UHPLC-MS
- Solvents, additives and blends for LC-MS
- Solvents for HPLC gradient
- Solvents for HPLC isocratic
- Solvents for HPLC preparative
- Mobile phases
- Silica gel and filter aids



SOLVENTS FOR UHPLC-MS

The UHPLC-MS is certainly the chromatographic technique for users who, besides being on the lookout for the best analytical performances, work at very high pressure, with minimum solvent consumption and need a guarantee of resolution and reproducibility of results.

In order to always be in line with the needs of its market and to provide the best service to our customers in term of quality and breadth of its range, CARLO ERBA Reagents has developed a specific range of solvents dedicated to solvents for UHPLC-MS in order to meet the quality requirements of this refined analytical technique.

- Purity higher than 99.99 %
- High UV transmission
- Excellent baseline quality in gradient tested specifically for UHPLC
- Reserpine test (< 30 ppb) => specific test for MS application
- Low content in inorganic and metallic ions
- Non volatile residue less than 1 ppm
- Filtration at least 0.2µm or 0.1µm
- Packaged in 1.1-difluoroethane treated amber glass to reduce significantly the potential formation of metals adducts

CODE : 412040			
CODE . 412040		MOLECUL	AR WEIGHT :41.05
CAS N° : 75-05-8			
FORMULA: CH3CN			
rest		U.M.	SPECIFICATION
Description			Clear colourless liquid
Colour		APHA	<= 5
dentification (I.R.)		-	Positive
Refractive index at 20°C			1.342 - 1.346
Residue on evaporation		ppm	<= 1
Acidity		meq/g	<= 0.0003
Alcalinity		meq/g %	<= 0.0002 >= 99.99
Assay (GC)			>= 99.99 <= 100
Nater (K.F.) JV Transmittance		ppm	<= 100
at 191 nm		%	>= 40
at 195 nm		%	>= 80
at 200 nm		%	>= 95
at 215 nm		%	>= 97
rom 230 nm		%	>= 99
JV Absorbance			-
at 191 nm		AU	<= 0.4
at 200 nm		AU	<= 0.03
at 220 nm		AU	<= 0.01
at 254 nm		AU	<= 0.005
Ruorescence (quinine)		-	-
at 254 nm		ppb	<= 1
at 365 nm		ppb	<= 0.5
at 450 nm	1	ppb	<= 0.5
JHPLC gradient peak at 210 nm		mAII	- <= 0.4
at 210 nm at 254 nm		mAU mAU	<= 0.4 <= 0.2
at 254 nm Gradient baseline drift at 210 nm		mAU mAU	<= 0.2 <= 6
Gradient baseline drift at 210 nm Gradient baseline drift at 254 nm		mAU mAU	<= 6 <= 2
Fest LC-MS TIC (50-2000m/z) ESI (+)	'		
Sensitive Impurities (reserpine)		ppb	<= 30
Vetals compounds			-
AI		ppb	<= 20
 Fe		ppb	<= 20
Na .		ppb	<= 50
Ca		ppb	<= 50
Мg	1	ppb	<= 20
C JV cut off 190 nm Metals compounds : mesured at batch re		ppb	<= 50
wetals compounds : mesured at batch re Filtered through a 0.1 µm membrane.	rease		

Product	Quality	UHPLC Gradient	Drift UHPLC	Pkg	Code
Acetonitrile	UHPLC-MS	At 210 nm <= 0.4 mAU	At 210 nm <= 6 mAU	1 L	412041
		At 254 nm <= 0.2 mAU	At 254 nm <= 2 mAU	2,5 L	412042
Methanol	UHPLC-MS	At 220 nm <= 4 mAU	At 220 nm <= 30 mAU	<u>1 L</u>	414941
		At 235 nm <= 2 mAU	At 235 nm <= 10 mAU	2,5 L	414942
		At 254 nm <= 1 mAU			
Water	UHPLC-MS	At 210 nm <= 2 mAU	At 210 nm <= 3 mAU	1 L	412091
		At 254 nm <= 0.5 mAU	At 254 nm <= 30 mAU	2,5 L	412092



SOLVENTS, ADDITIVES AND BLENDS FOR LC-MS

For your LC-MS routine analysis, CARLO ERBA Reagents offers a complete range of products with the most common solvents, additives and solutions ready-to-use among the most used mobile phases that bring you:

- Time saving
- Precise composition
- The assurance of an LC-MS quality
- Traceability
- Repeatability

Produced from LC-MS quality solvents and specifically tested for LC-MS coupling, these solutions guarantee :

- Test in gradient mode
- High UV transmission
- Solvent purity > 99.95 %
- Precise additive content
- Low content in inorganic and metallic ions
- Packaged in 1.1-difluoroethane treated amber glass to reduce significantly the potential formation of metals adducts

	Product	Quality	Pkg	Code
	Acetonitrile	LC/MS	1 L	412341
			2,5 L	412342
	Ethyl acetate	LC/MS	1 L	448383
v			2,5 L	448384
Solvents	Methanol	LC/MS	1 L	414831
Solv			2,5 L	414832
	Propanol-2	LC/MS	1 L	415183
			2,5L	415184
	Water	LC/MS	1 L	412111
			2,5 L	412112
	Acetic acid	LC/MS	10 x 1 ml	401411
			10 x 2,5 ml	401412
			50 ml	401413
	Ammonium acetate	LC/MS	50 g	418781
ives	Ammonium formate	LC/MS	50 g	419741
Additives	Formic acid	LC/MS	10 x 1 ml	405821
Αc			10 x 2,5 ml	405822
			50 ml	405823
	Trifluoroacetic acid	LC/MS	10 x 1 ml	411541
			10 x 2,5 ml	411542
			50 ml	411543
	Acetonitrile + 0.1% v/v formic acid	LC/MS	1 L	412331
			2,5 L	412332
	Acetonitrile + 0.1% v/v trifluoroacetic acid	LC/MS	1 L	412321
v			2,5 L	412322
Blends	Methanol + 0.1% v/v formic acid	LC/MS	1 L	414861
18			2,5 L	414862
	Méthanol + 0.1% v/v trifluoroacetic acid	LC/MS	1 L	414871
			2,5 L	414872
	Water+ 0.1% v/v formic acid	LC/MS	1 L	412121
			2,5 L	412122





SOLVENTS FOR HPLC GRADIENT


CARLO ERBA Reagents proposes 2 ranges : HPLC GOLD Ultragradient and HPLC PLUS Gradient for your analysis in Gradient mode.

The gradient control of elution and drift at critical wavelengths of our HPLC solvents Gold and Plus guarantee a peak free baseline. Their optimal sensitivity allows you to evaluate in the best possible way the impurities of your samples.

To make sure that no particle in the mobile phase will hinder your analyses, we carry out a microfiltration of our GOLD solvents at 0.1 μ m and for HPLC Gradient Plus at 0.2 μ m.

Product	Quality	Pkg	Code
Acetonitrile	HPLC Gold Ultragradient	1 L 4	12371000
		2,5 L 4	12372000
		4 L	412374
		5 L	412375
	HPLC Plus Gradient	1 L 4	12391000
	ACS-Reag.Ph.EurReag.USP	1 L*	412393
		2,5 L 4	12392000
Ethanol	HPLC Plus Gradient	1 L	4127012
		1 L*	4127032
		2,5 L	4127022
Methanol	HPLC - Gold Ultragradient	1 L	412721
		2,5 L	412722
		4 L	412724
		5 L	412725
	HPLC Plus Gradient	1 L	412381
		2.5 L	412383
Propanol-2	HPLC Plus Gradient	1 L 4	12711000
		2,5 L 4	12712000
Water	HPLC Plus Gradient	1 L	412141
		2,5 L	412142

	-
	412391000
VIII I	Acetonitrie
CAME	Assessment
a	UN 1648
1	

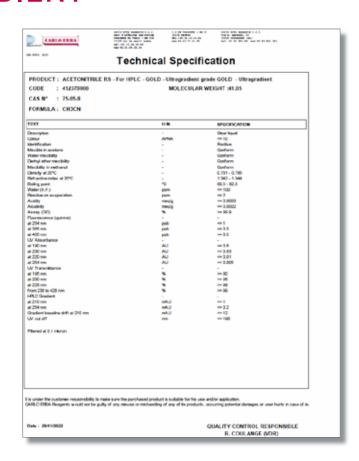



^{*} Glass bottle PVC coated

SPECIFICATIONS

			Acetonitrile			Methanol	
		UHPLC MS	LC MS	GOLD	UHPLC MS	LC MS	GOLD
		412040	412340	UltraGradient 412370000	414940	414830	UltraGradient 412720
Durity (CC)	%	min 00 00			min 00 00		
Purity (GC)		min 99.99	min 99.95	min 99.9	min 99.99	min 99.95	min 99.9
Water content	ppm	max 100	max 100	max 100	max 200	max 200	max 200
Non volatil residue	ppm	max 1	max 2	max 2	max 1	max 2	max 5
Acidity	meq/g	max 0.0003	max 0.0003	max 0.0003	max 0.0003	max 0.0003	max 0.0003
Titrable base Absorbance	meq/g	max 0.0002	max 0.0002	max 0.0002	max 0.00006	max 0.00006	max 0.0006
	A 11						
at 190 nm	A.U.	0.4		max 0.6			
at 191 nm	A.U.	max 0.4					
at 200 nm	A.U.	max 0.03		max 0.03			
at 220 nm	A.U.	max 0.01		max 0.01			
at 254 nm	A.U.	max 0.005		max 0.005			
UV Transmission (1cm -							
at 191 nm	%	min 40					
at 195 nm	%	min 80	min 80	min 80			
at 197 nm	%						
at 200 nm	%	min 95	min 95	min 95			
at 210 nm	%				min 40	min 30	min 30
at 215 nm	%	min 97					
at 220 nm	%		min 98				min 55
at 225 nm	%			min 99	min 70	min 65	min 65
from 230 nm	%	min 99	min 99	min 99			
from 240 nm							
at 235 nm	%			min 80		min 85	min 85
at 240 nm	%						min 90
at 250 nm	%					min 95	min 95
from 260 nm	%				min 98	min 98	min 98
Fluorescence (quinine) at 254 nm	ppb	max 1	max 1	max 1	max 1	max 1	max 1
Fluorescence(quinine) at 365 nm	ppb	max 0.5	max 0.5	max 0.5	max 1	max 1	max 1
Fluorescence (quinine) at 450 nm	ppb	max 0.5		max 0.5			
UHPLC gradient							
at 210 nm	mAU	max 0.4					
at 220 nm	mAU				max 4		
at 235 nm	mAU				max 2		
at 254 nm	mAU	max 0.2					
HPLC gradient	10	0.2					
at 210 nm	mAU		max 1	max 2			
at 235 nm	mAU		IIIGA I	IIIGA Z		max 2	max 2
at 254 nm	mAU		max 0.2	max 0.8		max 1	max 1
Drift at 210 nm	mAU	max 6	mg/, U.Z	max 12		IIION I	IIIUA I
Drift at 220 nm	mAU	IIIdA U		ΠΙΟΛ ΤΖ	max 30		
Drift at 235 nm	mAU						
	mAU	may 2		may 1	max 10		
Drift at 254 nm		max 2		max 1			
LC/MS test TIC (50-200	U (11/2) ESI (+)						
Sensitive impurities (in reserpine)	ppb	max 30	max 50		max 30	max 50	
Metal content (1):	ما مدمر	may 20	may F0		may 20	may FO	
Aluminium	ppb	max 20	max 50		max 20	max 50	
Iron	ppb	max 20	max 50		max 20	max 50	
Sodium	ppb	max 50	max 50		max 50	max 50	
Calcium	ppb	max 50	max 50		max 50	max 50	
Magnesium	ppb	max 20	max 50		max 20	max 50	
Potassium	ppb	max 50	max 50		max 50	max 50	

(1) Concentrations measured at batch release

SOLVENTS FOR HPLC ISOCRATIC

Available in glass bottles (1L and 2.5L) or stainless steel shuttle drums (5 to 1000L), their characteristics satisfy the requirements of the most advanced HPLC techniques in terms of purity and optical transmission.

Product	Pkg	Code
Acetic acid	1 L	401431
	2,5 L	401432
Acetone	1 L	412501
	2,5 L	412502
Acetonitrile	1 L	412411000
	2,5 L	412412000
Butanol	1 L	412511000
	2,5 L	412512000
1-Chlorobutane	1 L	431821
Chloroform stabilized with amylene	1 L	412571
	2,5 L	412572
Chloroform stabilized with ethanol	1 L	412652
	2,5 L	412653
Cyclohexane	1 L	412431000
	2,5 L	412432000
sym-Dichloroethane	1L	447191
	2,5 L	447192
Dichloromethane stabilized with amylene	1 L	412621000
	2,5 L	412622000
Dichloromethane stabilized with ethanol	1 L	412662
	2,5 L	412661
Dimethylformamide	1 L	444981
	2,5 L	444982
Dimethylsulfoxyde	1 L	445141
	2,5 L	445142
1,4 - Dioxane	1L	443231
Ethanol absolute anhydrous	1 L	4125212
	2,5 L	4125222
Ethanol 96	1 L	4145412
	2,5 L	4145422
Ethyl ether not stabilized	1 L	412671
	2,5 L	412672
Ethyle acetate	1 L	412611000
		412612000
n-Heptane 99%	1 L	412591000
	2,5 L	412592000
n-Heptane	1 L	446831
	2,5 L	446832



Product	Pkg	Code
Hexane 99 %	1 L	412691
	2,5 L	412692
n-Hexane		12601000
	2,5 L 4	12602000
Hexane Mixture of isomers	1 L	412632
	2,5L	412631
Isohexane	1 L	445152
	2,5 L	445151
Isooctane	1 L 4	12441000
	2,5 L 4	12442000
Methanol	1 L	412533
	1 L*	412531
	2,5 L	412532
	2,5 L*	412535
2-Methyltetrahydrofuran	1 L	412681
	2,5 L	412682
n-Pentane	1 L	P0643716
	2,5 L	P0643721
Propanol-1	1 L 4	12541000
	2,5 L 4	12542000
Propanol-2	1 L 4	12421000
	2,5 L 4	12422000
Ter-butylmethylether	1 L	432031
	2,5 L	432032
Tetrahydrofuran not stabilized	1 L 4	12451000
	_1L *. 4	12453000
	2,5 L 4	12452000
Tetrahydrofuran stabilized	<u>1 L</u>	412471
	2,5 L	412472
Toluene	1L 4	12641000
	2,5 L 4	12642000
Triethylamin	1 L	489631
	2,5 L	489633
* Glass bottle PVC coated		

Glass bottle PVC coated

SOLVENTS FOR HPLC PREPARATIVE

Our range of solvents for HPLC preparative have been designed to satisfy the requirements for separations and purifications. Their low non volatile residue content (5 ppm maximum) allows to optimize the operation conditions and to make impurity-free preparations.

All of these solvents are available in 2.5 L bottles and in stainless steel shuttle drums from 5 to 1 000 L.

Product	Code 2.5 L
Acetonitrile	412409
Chloroform stabilized with ethanol	438641
Dichloromethane stabilized with amylene	463281
Dichlorométhane stabilized with ethanol	463291
Ethyle acetate	448211
Propanol-2	415112
Tetrahydrofuran	487352
Ter-butylmethylether	432022000
Toluene	488531



TAILOR MADE SERVICE



All of our solvents for HPLC Preparative, Isocratic, Gradient, Ultragradient, LC-MS and eluant phases are also available in stainless steel shuttle drums from 5, 10, 25, 200 litres with sampling systems adapted to your needs.



SILICA GEL AND FILTER AIDS

CARLO ERBA Reagents proposes a wide range of silica gel among the general used types. Besides the widely used silica gel, other products with particular characteristics are also available and offer a series of valid alternatives for resolving numerous separation problems.

Product	Pkg	Code
Aluminum oxide (acid)	250 g	417185
	1 kg	417182
Aluminum oxide (basic)	100 g	417214
	1 kg	417217
Aluminum oxide (neutral)	250 g	417245
	1 kg	417241
	2.5 kg	417248
Aluminum oxide activated	1 kg	312261
Calcium carbonate	250 g	433245
Cellulose, powder	250 g	436061
Charcoal activated	250 g	434455
	1 kg	434454
Dicalite 4158	500 g	P8880014
	1 kg	P8880017
	5 kg	P8880027
Florisil 100-200 mesh	100 g	452351
	500 g	452353
Florisil 60-100 mesh for chromatography	100 g	452331
	500 g	452333
	1 kg	452332
Florisil 60-100 mesh for pesticides analysis	100 g	452271
	500 g	452273
Kieselguhr composed	250 g	449895
	250 g	449897
Magnesium oxide	1 kg	459617
Sand purified	1 kg	477153



Product	PKg	Code
Silica gel 60A 6 - 35µ	1 kg	P2010017
	5 kg	P2010027
	25 kg	P2010044
Silica gel 60A 20 - 45µ	1 kg	P2200017
	5 kg	P2200027
Silica gel 60A 35 - 70µ	1 kg	P2000017
	2 kg	P2000026
	5 kg	P2000027
	25 kg	P2000044
Silica gel 60A 40 - 63µ	1 kg	P2050017
	5 kg	P2050027
	25 kg	P2050044
Silica gel 60A 70 - 200µ	1 kg	P2100017
	2 kg	P2100026
	5 kg	P2100027
	25 kg	P2100044
Silica gel 60A 0,06÷0,20 mm	500 g	453336
	1 kg	453337
	5 kg	453332
	20 kg	453331



MOBILE PHASES

If you regularly use an eluent phase, we can prepare it for you according to your specifications.

Your mobile phase is prepared from HPLC quality solvents according to procedures (respect of the GMPs) and with validated equipment in compliance with your specifications or a pharmacopeia.

The ready-to-use eluent phase provides you with:

- Important time saving for preparation
- Reduction of risks linked to the handling of toxic or hazardous products
- Guaranteed pH
- Possibility of large sized homogeneous batches
- Labelling conforming to legislation and to BPLs

It is supplied with:

- Certificate of analysis of the batch
- Safety data sheet

Examples

Acetonitrile + methanol + buffered pH 3

Acetonitrile + water

Ethyl acetate + toluene

Batch number RE-TEST date


Water + TFA

Water + THF

Specifications defined by customer

Composition

Date

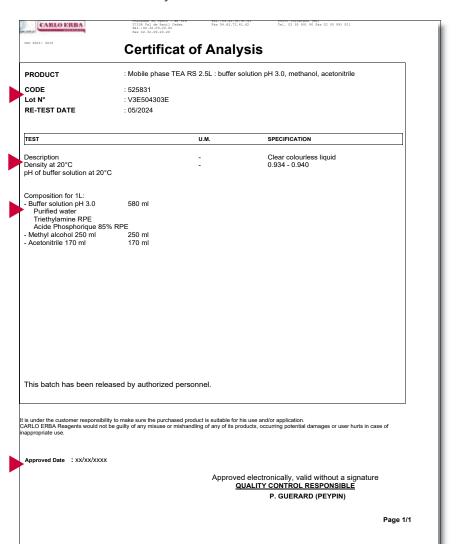



Tailor made

Chemicals such as you imagine



CARLO ERBA Reagents thanks to its experience and production flexibility manufacture tailor made products for industry and laboratories.



- Custom mixture
- Purification
- Custom packaging
- Deliveries in bulk tanks and isotanks
- Shuttle service
- Analytical control
- Batch management
- Quality assurance

www.carloerbareagents.com

GAS CHROMATOGRAPHY

Broad spectrum chemical analysis of trace level components is a continuing challenge for any analytical chemist. This challenge is further confounded when chemical impurities may be present in common organic solvents or when chemical artifacts may be formed, produced and introduced during an analytical procedure. Minimizing and understanding these chemical artifacts is critical for trace level detection and is crucial for accurate analytical conclusions.

CARLO ERBA Reagents GC Solvents are the right choice for your complex mixture challenges.



ANALYSIS METHOD

GC-FID GC-ECD GC-Headspace GC-MS For analysis of organic substances For analysis of For residual For high sensitivity and trace of pesticides and solvents anakysis analysis hydrocarbons chlorinated in pharmaceutical substances industry RS - ATRASOL® RS - PESTIPUR® **RS - HEADSPACE** RS - GC-MS

In this brochure, we offer you a choice of products specifically adapted for the preparation and analysis of your samples by GC :

CARLO ERBA Reagents GRADES

- Solvents for HEADPSACE
- ATRASOL® Solvents for the detection of traces in organic compounds and hydrocarbons
- ATRASOL® Solvents for Hydrocarbon index determination according to EN ISO 9377-2
- Solvents for GC-MS
- PESTIPUR® Solvents for pesticides residue analysis
- Organic standards



HEADSPACE SOLVENTS

The International Conference on Harmonization (ICH) adopted a document named "impurities": this is an explicative note related to residual solvents, which prescribes the maximum amount of solvent in active substances, excipients, and medications after their synthesis. The methods used for their identification are described in the chapters 467 of USP and 2.4.24 of the European pharmacopeia.

Three classes of solvents are defined:

- Class 1 : Solvents to be avoided.
- Class 2 : Solvents to be limited
- Class 3 : Solvents with low toxic potential

The technique used to determine these Organic Volatile Impurities (OVI) is GC-Headspace which requires the use of organic solvents to dissolve and/or extract the sample. These solvents need to be free of impurities that could interfere with the GC trace.

CARLO ERBA Reagents offers a **specific product line** dedicated to the GC-Headspace technique. Utilizing our solvents developed and tested specifically for GC-headspace ensure the highest quality and batch to batch consistency for your tests.





Product	Pkg	Code
n,n-Dimethylacetamide	1 L	444311
n,n-Dimethylformamide	1 L	444991
Dimethylsulphoxide	1 L	445121
n-Methylpyrrolidone-2	1 L	462881
Water	1 L	412011

REFERENCE STANDARDS FOR ANALYSIS OF RESIDUAL SOLVENTS

CARLO ERBA Reagents developed a range of solvent mixtures class 1 and 2, with concentration within the allowable limits established in chapter 467 of the USP and 2.4.24 of the European Pharmacopeia. These mix allow you to determine the amount of residual solvents in your raw material that can be used for API synthesis.

All the standards come with certificate of analysis insuring total traceability :

- Batch number and expiration date
- CAS number of each component
- Molecular formula of each component
- Batch number of each bulk material used
- Concentration of each component
- Expanded uncertainties

Solvents type	Pkg	Code
Mix (Recommended by European Pharmacopeia / ICH class 1): 5 elements	Sealed ampule 1 mL	507688
Mix (Recommended by USP < 467 > class 1): 5 elements	Sealed ampule 1 mL	507692
Mix 1 (Recommended by European Pharmacopeia / ICH class 2): 14 elements	Sealed ampule 1 mL	507689
Mix 2 (Recommended by European Pharmacopeia / ICH class 2): 11 elements	Sealed ampule 1 mL	507690
Mix 3 (Recommended by European Pharmacopeia / ICH class 2): 6 elements	Sealed ampule 1 mL	507691
Mix 1 (Recommended by USP < 467 > class 2): 16 elements	Sealed ampule 1 mL	507693
Mix 2 (Recommended by USP < 467 > class 2): 6 elements	Sealed ampule 1 mL	507694



ATRASOL® SOLVENTS FOR THE DETECTION OF TRACES IN ORGANIC COMPOUNDS AND HYDROCARBONS

Rigorous gas chromatographic controls and extreme operation accuracy in both production and packaging make these the best-suited solvents in gas chromatography for all determinations of traces of organics requiring extreme precision and sensitivity.

High purity, guaranteed absence of extraneous peaks in gas chromatographic determinations and guarantee of reproducibility and repeatability of the results are the main feature of this product line.

For the entire **ATRASOL®** line, the absence of critical impurities is ensured by means of precise functionality tests in **GC-ECD** and **GC-FID**.

Refractive index at 20°C - 1,327 · 1,331 Water (K.F.) ppm <300 Residue on evaporation ppm <2 Colour APHA <5 Free acid (as HCDOH) ppm <10 Free acid (as HCDOH) ppm <1 Free acid (as HCDOH) ppm <1 Assay (CC) % >99.98 GC-ECD.Individual peak (Indrahe) μg/L <1 Ret. range dichloromethane - - to 1,24 trichlorobenzene - - to decachlorobiphenyle - - GC-ED.Individual peak (in-hexadecane) μg/L <2 Ret. range n-undecane to n-tetracontane - - This batch has been released by authorized personnel. - -			Specificat		
Lot N° : ΧΧΧΧΧΧΧΧΧ CAS N° : 67-56-1 FORMULA : CH3OH TEST U.M. SPECIFICATION Description - Clear colourless liquid Refractive index at 20°C - 1.327 - 1.331 Refractive index at 20°C - 1.327 - 1.331 Residue on evaporation ppm < 30	PRODUCT	: Methanol RS A	FRASOL For trace	analysis	
RE-TEST DATE ∴ xx/xxxx CAS N° : 67-56-1 FORMULA : CH3OH ITEST U.M. SPECIFICATION Description Refractive index at 20°C - 1.327 · 1.331 Water (K.F.) ppm < 300 Residue on evaporation ppm < 2 Colour APHA < 5 Free acid (as HCOOH) ppm < 10 Free acid (as HCOOH) ppm < 10 Free alidi (as WH3) ppm < 10 Free alidi (as WH3) ppm < 1 Ret.range dichloromethane - - to 1,2,4 trichlorobenzene - - CC-ED.Individual peak (Lindane) ng/L < 2 Ret.range 1,2,4 trichlorobenzene - - GC-ED.Individual peak (In-hexadecane) µg/L < 2 GC-FID.Individual peak (In-hexadecane) µg/L < 2 Ret. range n-undecane to n-tetracontane - - This batch has been released by authorized personnel. <th></th> <th></th> <th></th> <th></th> <th></th>					
CAS N° : 67-56-1 FORMULA : CH3OH TEST U.M. SPECIFICATION Description - Clear colourless liquid Refractive index at 20°C - 1.327 - 1.331 Water (K.F.) ppm <= 300 Residue on evaporation ppm <= 2 Colour APHA <= 5 Free acid (as HCOOH) ppm <= 10 Free asidial (as NH3) ppm <= 10 Free asidial (as NH3) ppm <= 1 GC-ECI.ndividual peak (CCI4) μg/L <= 1 Retrange (Inchirormethane - - to 1,24 trichlorobenzene - - CC-ECI.ndividual peak (Indane) ng/L <= 2 Retrange 1,24 trichlorobenzene - - to decachiorobiphenyle - - GC-FID.Individual peak (In-hexadecane) μg/L <= 2 Ret. range n-undecane to n-tetracontane - - This batch has been released by authorized personnel. Is under the customer responsibility to make s	Lot N°				
TEST	RE-TEST DATE	: xx/xxxx	M	OLECULAR WEIGHT: 32,04	
TEST	CAS N°	: 67-56-1			
Description - Clear colourless liquid	FORMULA	: CH3OH			
Refractive Index at 20°C - 1.327 · 1.331 Residue on evaporation ppm <= 3	TEST		U.M.	SPECIFICATION	
Refractive Index at 20°C	Description		-	Clear colourless liquid	
Residue on evaporation Colour APHA C=5 Free acid (as HCCOH) Free alcid (as HCCOH) Ppm					
Colour APHA < 5 Free acid (as HCOOH) ppm <= 10 Saxay (CC) % >= 99.98 GC-ECD.Individual peak (LICIA) μg/L <= 1 Fet trange (1.2 A trichloroberzene CC-ECD.Individual peak (Lindane) ng/L <= 2 GC-ECD.Individual peak (Indane) ng/L <= 2 GC-ED.Individual peak (In-hexadecane) μg/L <= 2 GC-FID.Individual peak (n-hexadecane) μg/L <= 2 Ret. range n-undecane to n-tetracontane			ppm	<= 300	
Free aid (as HCOOH)				<= 2	
Free alkali (as NH3) ppm <=1 Sasay (GC) % >=99.98 GC-ECD.Individual peak (CCI4) μg/L <=1 GC-ECI.Ondividual peak (Indane) ng/L <=2 GC-ECI.Ondividual peak (Indane) ng/L <=2 GC-ECI.Ondividual peak (Indane) ng/L <=2 GC-ED.Individual peak (Indane) ng/L <=2 GC-ED.Individual peak (Indane) ng/L <=2 GC-FID.Individual peak (n-hexadecane) μg/L <=2 GC-FID.Individual peak (n-hexadecane) μg/L <=2 This batch has been released by authorized personnel.	Colour		APHA	<= 5	
Assay (CC) % >= 99.98 GC-ECD.Individual peak (CCI4) μg/L <= 1 Ret.range dichloromethane	Free acid (as HCOOH)		ppm	<= 10	
GG-ECD.Individual peak (CICI4) μg/L <= 1 Ret.range dichloromethane					
Ret. range dichloromethane					
to 1,24 frichlorobenzene G-G-ECD.Individual peak (Lindane) Ret.range 1,24 frichlorobenzene 1 of decachlorobiphenyle GC-FID.Individual peak (n-hexadecane) Ret. range n-undecane to n-tetracontane This batch has been released by authorized personnel. Is under the customer responsibility to make sure the purchased product is suitable for his use and/or application. ARAID STBAR Reagents would not be guilty of any misuse or mishandling of any of its products, occurring potential damages or unter in case of appropriate use.			μg/L	<= 1	
GC-ECD individual peak (Lindane) Ret.range 1.2 At richisrobenzene to decachlorobiphenyle GC-FID. Individual peak (In-hexadecane) Ret. range 1.2 At richisrobenzene			-	-	
Ret. range 1,2,4 trichforobenzene			-	•	
to decachlorobiphenyle GCF-FD.Individual peak (n-hexadecane) µg/L <= 2 Ret. range n-undecane to n-tetracontane			ng/L	<= 2	
GC-FID.Individual peak (n-hexadecane) μg/L <= 2 Ret. range n-undecane to n-tetracontane - This batch has been released by authorized personnel. Is under the customer responsibility to make sure the purchased product is suitable for his use and/or application. ARLO ERBA Reagents would not be guilty of any misuse or mishandling of any of its products, occurring potential damages or unspropriete use.				•	
Ret. range n-undecane to n-tetracontane This batch has been released by authorized personnel. Is under the customer responsibility to make sure the purchased product is suitable for his use and/or application. ARLO ERBA Reagents would not be guilty of any misuse or mishandling of any of its products, occurring potential damages or urst in case of appropriate use.				* .	
This batch has been released by authorized personnel. Is under the customer responsibility to make sure the purchased product is suitable for his use and/or application. ARLO ERBA Reagents would not be guilty of any misuse or mishandling of any of its products, occurring potential damages or utrain case of appropriate use.			μg/L	<= 2	
is under the customer responsibility to make sure the purchased product is suitable for his use and/or application. ARILO ERBA Reagents would not be guilty of any misuse or mishandling of any of its products, occurring potential damages or use in case of appropriate use. Approved Date: xx/xx/xx/xxxxx	This batch has been rele	ased by authorized pe	ersonnel.		
Approved Date : xx/xx/xxxxx	ARLO ERBA Reagents would urts in case of				or user
Approved Date : xx/xx/xxxx					
	Approved Date : XX/XX/XX	**			
Approved electronically, valid without a signatu QUALITY CONTROL RESPONSIBLE					ture
P. GUERARD (PEYPIN)					

Product	Pkg Code
Acetone	1 L P0053216
	2,5 L P0053222
	4 L P0053282
Chloroform stabilized with ethanol	1 L P02432E16
	2,5 L P02432E21
Dichloromethane stabilized with amylene	1 L P02932A16
	2,5L P02932A21
	4 L P02932A82
Dichloromethane stabilized with ethanol	1 L P02932E16
	2,5 L P02932E21
n,n-Dimethylformamide	1 L P0343216
	2,5 L P0343221
Dimethylsulphoxide	1 L P0353216
	2,5 L P0353221
Ethyl acetate	1 L P0023216
	2,5 L P0023221
n-Hexane 99%	1 L P052323016
	2,5 L P05232302
Methanol	1 L P0933216
	2,5 L P0933221
n-Pentane 99%	1 L P064323016
	2,5 L P06432302
Toluene	1 L P0713216
	2,5 L P0713221
	4 L P0713282



ATRASOL® SOLVENTS FOR HYDROCARBON INDEX DETERMINATION ACCORDING TO EN ISO 9377-2

The European regulation **EN ISO 9377-2** "Determination of hydrocarbon oil index - Method using solvent extraction and gas chromatography", established the criteria for the evaluation of the hydrocarbon index in water using gas chromatography. This procedure is suitable for surface water, wastewater and water from sewage treatment plants.

Isohexane, hexane and petroluem ether ATRASOL®, with their boiling range between 36 and 69 °C, are ideal for this application. Each batch is specifically analyzed so that the hydrocarbon index is less than or equal to 0.1 mg/l, in the retention time window between n-decane and n-tetracontane.

Product	Pkg	Code
n-Hexane	1 L	P0523216
	2,5 L	P0523221
Isohexane	1 L	P6263216
	2,5 L	P6263221
n-Pentane	1 L	P0643216
	2,5L	P0643221
Petroleum ether 35 - 60°C	1 L	P0883216
	2,5 L	P0883221

CALAD FIRE | Section | Sec

REFERENCE STANDARDS

For the determination of mineral oils, the regulation prescribes specific mixtures of standard solutions. CARLO ERBA Reagents has a complete range of standard mixtures, each with a certificate of analysis with complete information on the composition and gravimetric validation carried out in reference to NIST standards.

Product	Pkg	Code
Standard quality control of 2 mineral oils in acetone 0.5mg/ml each	1 mL	506002
Mixture of 2 mineral oils without additive 5 mg / ml each in hexane	1 mL	506010
	5 mL	506012
	10 mL	506013
Mixture of 2 mineral oil without additive 1 mg/ml each in hexane	10 mL	506011
Standard mixture of n-alkanes (C10 to C40 in pairs) of 50 µg/ml each in hexane	1 mL	506020
	10 mL	506021
Mother solution of extraction solvent: N-tetracontane mixture (20 mg/l) and n-decane (20 µg/l) in hexane	5 mL	506040
Test solution stearyl stearate 2 g / l in hexane	10 mL	506030

GC-MS SOLVENTS

The birth of the gas chromatogram coupled to a mass spectrometer in the early 1950's allowed the utilization of 2 technologies for the fast qualitative and quantitative determination of samples. Gas chromatography allows the separation of components in a mixture and mass spectroscopy the characterization of the identified components. Over the years, several type of mass spectrometers were coupled to a GC such as quadrupoles, ion traps and time of flight allowing for more accurate results depending on the type of samples analyzed. The evolution of the technology by the different manufacturers over the years resulted in lower detection and quantitative limits. More recently, an increase of the use and applications of 2D GC-MS has been witnessed. This technology dating back from the early 1990's gives an increase peak capacity of the GC allowing for the analysis of more complex mixtures.

Furthermore, the complexity of the samples commonly encountered for the analysis of volatile substances, and the achievement of the increasingly restrictive analytical sensitivities required by international regulations, make the interpretation of the data critical for the reliability of the final result.

The recent technological advances of GC-MS, GC-MS/MS and 2D GC-MS have opened new analytical horizons, in terms of selectivity of the result, and allowed a reduction of detection limits, reducing the need for cleaning the sample and the introduction of faster methods for sample preparation.

Product	Pkg	Code
Acetone	1 L	400952
Chloroform stabilized with ethanol	1 L	438732
Dichloromethane stabilized with amylene	1 L	463342
Dichlorométhane stabilized with ethanol	1 L	463332
Ethyl acetate	1 L	448342
n-Hexane 99 %	1 L	447212
Methanol	1 L	414952
n-Pentane 99%	1 L	468172
n-Pentane	1 L	468182

The role and the choice of the quality of the solvent is consequently crucial for the production of a precise and accurate analytical data. That is why we are introducing a new product range dedicated to the most demanding need for GC-MS. These products were specifically tested for GC/MS test for individual signals, with a retention range of C_{11} to C_{40} with a scanning area of 30-600 amu with a guarantee of less than $2\mu g/l$ of impurities.

The CARLO ERBA Reagents GC-MS solvents guarantee excellent performance, even for the analysis of the most complex mixtures. They are characterized by:

- Very high purity
- Extremely low non volatile residue content
- Functionality tested in GC-MS



PESTIPUR® SOLVENTS FOR PESTICIDES RESIDUE ANALYSIS

The control of pesticide residues in the food and environmental sectors is remarkably important today, as these substances represent a potential public health hazard. The purity of the solvent is a determinant factor in obtaining reliable results. Thus it is essential to have products available with suitable parameters for this type of application.

To meet these needs, CARLO ERBA Reagents offers its **PESTIPUR®** line of solvents, specific for the extraction of pesticides and the analysis of chlorinated and nitrogenous residues, even at trace levels. Our products are prepared according to the most advanced distillation techniques and strictly controlled in order to guarantee the highest level of quality.

Various functionality tests ensure a stable base line in gas chromatography. For the entire **PESTIPUR®** line, the absence of critical impurities is ensured by means of precise functionality tests in GC-ECD and GC-NPD.

Product	Pkg	Code
Acetone	1 L	400991
	2,5 L	400992000
Acetonitrile	1 L	401241
	2,5 L	401242
tert-Butylmethylether	1 L	432061
	2,5 L	432062
Chloroform stabilized with amylene	1 L	438681
	2,5 L	438682
Chloroform stabilized with ethanol	1 L	438651
	2,5 L	438652
Cyclohexane	1 L	436931
	2,5 L	436932
Dichloromethane stabilized with amylene	1 L	442291
	2,5 L	442292000
	4 L	442294
Dichlorométhane stabilized with ethanol	1 L	442261
	2,5 L	442262
Diethyl ether not stabilized	1 L	447651
	2,5 L	447652
Dimethylformamide	1L	444941
Ethyl acetate	1 L	448351
	2,5 L	448352000

Product	Pkg	Code
n-Heptane 99%	1 L	446951
	2,5 L	446952
Heptane mixture of isomers	1 L	446841
	2,5 L	446842
n-Hexane 99 %	1 L	447111
	2,5 L 4	47112000
n-Hexane	1 L	447011
	2,5 L	447012
	4 L	447013
Hexane Mixture of isomers	_1 L	447181
	2,5L	447182
Isohexane	1 L	447131
	2,5 L	447132
Isooctane	1 L	456791
	2,5 L	456792
Methanol	1 L	414930
	2,5 L	414932
n-Pentane	1 L	468161
	2,5 L	468162
Petroleum ether 40 - 65°C	1 L	447851
	2,5 L	447852
Petroleum ether 35 - 60°C	1 L	447862
	2,5 L	447861
Propan-2-ol	1 L	415281
Toluene	1 L	488591
	2,5 L	488592
	4 L	488594

ISO 17993:2002 specifies a method using high performance liquid chromatography (HPLC) with fluorescence detection for the determination of 15 selected PAHs in drinking and ground water in mass concentrations are greater than 0,005 μg/l (for each single compound) and surface waters in mass concentrations above 0,01 μg/l.

To avoid additional internal validation, CARLO ERBA Reagents tests the PAH content of Dichloromethane quality PESTIPUR® according to NF EN ISO 17993: 2002 and guarantees the minimum possible interference to use.

ORGANIC STANDARDS FOR RESIDUE ANALYSIS AND ENVIRONMENTAL ANALYSIS

CARLO ERBA Reagents offers the possibility to realize tailored formulations of organic substances (pesticides, IPA, PCB, nitrogenous substances, chlorinated, etc ...) produced according to an ISO 17025 accredited Quality Management System and ISO Guide 34.

Organic standard solutions are prepared according to your analytical needs for HPLC, GC and GC-MS. These solutions are custom-made standards which bring you lots of advantages:

- Time saving for preparing and controlling standard solutions
- Traceability to NIST
- Specific for instrument calibration
- No risk of precipitation mixing incompatible solutions: the best solution (two or more mixes or another solvent) is proposed if there's a problem of compatibility.
- Exact quantity needed (from 0.5 ml in ampules or CERTAN bottles to 500 ml)

Each of our products are delivered with a certificate of analysis including:

- Batch number
- Expiry date
- Storage information
- CAS number, formula, purity of each starting material
- Gravimetric data



						FOR CO. MICH. ACCRECATION
						FOR TO 98 75 ATSWEED
						FOR CO. SECTION SECTIO
						508 W MHS (100000)
						PORTAL MEDIANOSIS
						1.2.4 Frontierdaments Mr.Ph. per-Malein.
						Resolvant - 3 debatere (6.0% pright (6.0%) Resolvanterance (6.0% pright (6.0%)
						April 1071 St. Co. Landson
						Bear Co. But and Title
						Service Officialisms State (Francisco
						Separation the programme
						0.6560 g/m* d 21.3 °C
						play date: unit 04 2019
						miled year.
N	al Infor	mation				Editoratory Disk Only ECRS is intended for
c	netric D					DIRECTOR of T.C. GOFD, GOTCD, GOECD, GOMS, HPLOUV SHILLIPLONS
•	neeric L	/USA				Continue of analytical methods
						Superior of 'working reference samples'
	West Street	Fred.	200	Conne	Chemist	
	-		-	1000	-	Diffection land and trearly studies
	-	No. 17	National	1974		Editioned a not manded to restrict the use for other purposes.
			56.76			displaces for the correct use of this reference material.
п	1.000	8.75/No.	***	State ()	100	CONTRACT reference material can be used directly or can be discled in an appropriate actions.
	14,0740	11,000	ALC: NAME OF	76.675	200	III glasseure should be used. On not pipel from container: Obtained concentration (in regift of
	1400	DOM:	100000	1.079	270	Miguil from the multiplication of certified value of CRM concentration and the CRM's volume of
	+	1.000	Access to	1766.5	-	Bill and divided the fire facil's volume used for divisor.
	10.7607	11.500	10000	76.546	-	
						Billity and storage:
	4.66700	12.760	CHER	1.010	Ph.	BESTAL in with a guaranteed stability until affil. of the certified concentration for a period of \$6.0
	1876	1.0000	*100000	15764	100	this is purported of an unspecial ampoule as writen in description of the reference material
	4038	11,560	Control	19,777	200	IEEE's product is stable at normal laboratory conditions, in order to increase its atability, we have
,	14000	10.76	100000	1.564	200	attitioned it to be aboracl in a refrageration.
	4.6000	1.000	An investment	100.00	-0.0	Built should be used shortly after sparing to avoid concentration changes due to evaporation.
	10,7184	11.580	10400	70.000	PN .	BOM apply to ampoules stored after opening.
		11.76	1000	1.00		
	1.000				- 10	Selbon shadon
	1.0100	3.7860	100000	1999.1	100	
r	44,2000	13,5607	4Chest F	70.462	PN	
•	1400	11.70	100000	1.000	276	
	440077	1.000	Accession 6	delite i	40	
	m has	11.500	TOWARD !	75.604	PN .	
ì	1.000	10.70	1000	1.00	Pi	
	8.80000	1.66(1)	100000	1000.0	101	
۰	11.700()	11,560	4 Charles	70.676	PH1	
	1400	11.70	100408	1,404	270	
	0.000	5.0mm	ACTOR	Time	400	
	10.0700	11.000	10000	200	2764	
	4.00000	11.76	10000	1,000	200	
ŀ	1000	1.900	1000	200,40		
۰	6.675	13,5667	Carr	74.676	200	
•	1.60%	11.70	10000	1,756	270	
r	0.076	1.0100	407049	10074.6	400	
	0.000	11.3965	100407	75.00	2704	
	4 months	E1 760	10000	1.400	100	
ŀ	14000	1000	10000	19074	-	
	0.004	11,560	ACMINITY.	7.67	-	
•	1.4000	1.70	COMM	1,701	200	
	44.36	100000	40400	French.	-	
	8.756	11,000	TOTAL CO.	19,780	276	
	4.0000	10.760	107000	1.500	Ph.	
r	14700	1. class	110000	1000.0	100	
	0.000	13.560	ACCRECATE	70.000	-	
	1400	1.70	17767	100	-	
ŀ						
	4.61.00	1.60%	ALC: UNKNOWN	467.4		
	100	11,000	STREET, STREET,	71.65	27%	
	4 million	School Service		1.570	PRI	

Send us:

- CAS number
- Concentration
- Solvent
- Volume
- Packaging

to receive our best and most suitable offer according to your needs!



ION PAIR CHROMATOGRAPHY

Ion Pair Chromatography has been developed to allow the separation of complex mixtures of polar and ionic molecules, which often are not well separated by ion exchange chromatography. The selectivity is determined by the mobile phase: the organic eluent is supplemented with a specific ion-pairing reagent. The IPC reagents are large ionic molecules having a charge opposite to the targeted analyte, as well as an hydrophobic region to interact with the stationary phase. The counter-ions combine with the ions of the eluent, becoming ion pairs in the stationary phase. Ion pairs are then separated on Reverse-phase HPLC columns.

The purity of the mobile phase and therefore the accuracy of the results depends on the quality of the additive. The specifications of our ion pair reagents are in line with the requirements of Reverse-phase HPLC:

- High purity ≥ 99%
- Minimum UV absorption in the far UV
- Controlled pH
- Loss on drying

CARLO ERBA Reagents selected the most commonly used ion pair reagents (straight-chain alkyl sulfonic acids...and quaternary alkylated ammonium salts) for your basic samples :

Product	CAS number	Pkg	Code
1-Butanesulfonic acid sodium salt	2386-54-1	25 g	405631
		100 g	405632
1-Decanesulfonic acid sodium salt	13419-61-9	25 g	405871
		100 g	405872
1-Dodecanesulfonic acid sodium salt	2386-53-0	25 g	405881
		100 g	405882
Dodecyltrimethylammonium bromide	1119-94-4	25 g	405941
		100 g	405942
1-Heptanesulfonic acid sodium salt	22767-50-6	25 g	405851
		100 g	405852
1-Hexanesulfonic acid sodium salt	2832-45-3	25 g	405621
		100 g	405622
1-Hexanesulfonic acid sodium salt monohydrate	207300-91-2	25 g	405921
		100 g	405922
1-Octanesulfonic acid sodium salt	5324-84-5	25 g	405861
		100 g	405862
		1 kg	405863
1-Octanesulfonic acid sodium salt monohydrate	207596-29-0	25 g	405931
		100 g	405932
1-Pentanesulfonic acid sodium salt	22767-49-3	25 g	405841
		100 g	405842
1-Pentanesulfonic acid sodium salt monohydrate	207605-40-1	25 g	405891
		100 g	405892
1-Propanesulfonic acid sodium salt	14533-63-2	25 g	405901
		100 g	405902
Tetrabutylammonium bisulfate	32503-27-8	25 g	405971
		100 g	405972






ULTRAPUR / SUPERPUR acids for Trace Metal analysis





ION CHROMATOGRAPHY

Ion Chromatography is a widely used technique that separates ions and polar molecules based on their affinity to the ion exchanger. It is often used in protein purification and water analysis. It works on almost any kind of charged molecule - including large proteins, small nucleotides, and amino acids.

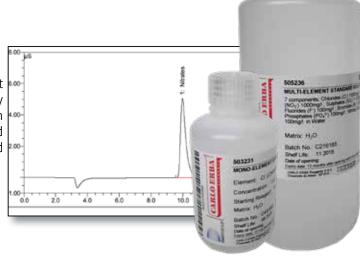

CONCENTRATED MOBILE PHASES

The following eluents are filtered at 0.2µm and prepared from ultra-pure salts and 18-megaohm deionized water. These are concentrated solutions that should be diluted by a factor of 100.

They are characterized by:

- Guaranteed titer with its uncertainty
- Raw materials selected and verified against N.I.S.T. Standard Reference Materials

- Available in HDPE bottles
- Certificate of analysis with references on the analytical method, the N.I.S.T. Standard Reference Materials and the confidence interval
- Shelf life, for the unopened product package, of 2 years.

Product		Pkg	Code
Eluent sodium bicarbonate	0.17 M Sodium bicarbonate	100 mL	504534
Eluent sodium bicarbonate	0.5 M Sodium bicarbonate	1 L	507578
Eluent sodium carbonate	0.1 M Sodium carbonate	1 L	507695
Eluent sodium carbonate	0.5 M Sodium carbonate	100 mL	504533
		1 L	507577
Eluent sodium carbonate/sodium bicarbonate	0.18 M Sodium carbonate /	100 mL	504530
	0.17 M Sodium bicarbonate		
Eluent sodium carbonate/sodium bicarbonate	0.22 M Sodium carbonate /	100 mL	504531
	0.28 M Sodium bicarbonate		
Eluent sodium carbonate/sodium bicarbonate	0.35 M Sodium carbonate /	100 mL	504532
	0.1 M Sodium bicarbonate		




STANDARD SOLUTIONS

Our standard solutions for ion chromatography are obtained by dissolution of a high-purity salt (+99.9%) in water.

They are characterized by:

- Concentrations equal to 1000 ppm
- Guaranteed titer with its uncertainty
- Raw materials selected and verified against N.I.S.T. Standard Reference Materials
- Available in HDPE bottles
- Certificate of analysis with references on the analytical method, the N.I.S.T. Standard Reference Materials and the confidence interval
- Shelf life, for the unopened product package, of 2 years.

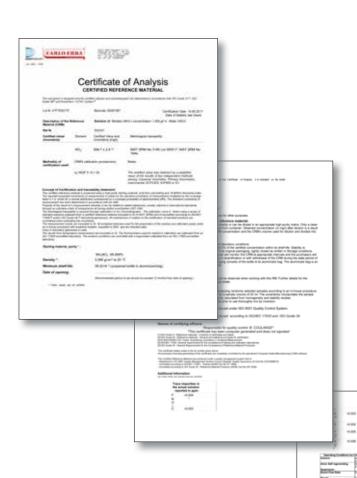

Product	Pkg	Code
Ammonium standard solution	100 mL	503311
conc. 1.000 ppm Matrix : Water	500 mL	503313
Bromate standard solution	100 mL	503171
conc. 1.000 ppm Matrix : Water	500 mL	503173
Bromide standard solution	100 mL	503211
conc. 1.000 ppm Matrix : Water	500 mL	503213
Calcium standard solution	100 mL	503221
conc. 1.000 ppm Matrix: Water and nitric acid	500 mL	503223
Chlorate standard solution	100 mL	503181
conc. 1.000 ppm Matrix : Water	500 mL	503183
Chloride standard solution	100 mL	503231
conc. 1.000 ppm Matrix : Water	500 mL	503233
Chlorite standard solution	100 mL	503191
conc. 1.000 ppm Matrix : Water	500 mL	503193
Chromate standard solution	100 mL	503241
conc. 1.000 ppm Matrix : Water	500 mL	503243
Cyanide standard solution	100 mL	503358
conc. 1.000 ppm Matrix : Water and nitric acid		
Fluoride standard solution	100 mL	503251
conc. 1.000 ppm Matrix : Water	500 mL	503253
lodide standard solution	100 mL	503261
conc. 1.000 ppm Matrix : Water	500 mL	503263
Lithium standard solution	100 mL	503281
conc. 1.000 ppm Matrix : Water	500 mL	503283
Magnesium standard solution	100 mL	503291
conc. 1.000 ppm Matrix: Water and nitric acid	500 mL	503293
Nitrate standard solution	100 mL	503331
conc. 1.000 ppm Matrix : Water	500 mL	503333
Nitrite standard solution	100 mL	503321
conc. 1.000 ppm Matrix : Water	500 mL	503323
Phosphate standard solution	100 mL	503271
conc. 1.000 ppm Matrix : Water	500 mL	503273
Potassium standard solution	100 mL	503221
conc. 1.000 ppm Matrix : Water	500 mL	503223
Sodium standard solution	100 mL	503301
conc. 1.000 ppm Matrix : Water	500 mL	503303
Strontium standard solution	100 mL	503361
conc. 1.000 ppm Matrix : Water		
Sulfate standard solution	100 mL	503351
conc. 1.000 ppm Matrix : Water	500 mL	503353



CUSTOMIZED STANDARD SOLUTIONS

CARLO ERBA Reagents offers the possibility to realize custom mixtures. It can be mono-element or multi-element. It brings you:

- Time saving for preparing and controlling standard solutions
- Traceability to NIST
- Specific for instrument calibration
- No risk of precipitation mixing incompatible solutions: the best solution (two or more mixes or another solvent) is proposed if there's a problem of compatiblity.
- Exact quantity needed (from 100 ml to 1l)

Each of our products are delivered with a certificate of analysis including:

- Batch number
- Expiry date
- Storage information
- CAS, formula, purity of each starting material
- Guaranteed titer with its uncertainty

Send us :

- Element
- Concentration
- Solvent
- Volume
- Packaging

to receive our best and most suitable offer according to your needs!



ERBAqua®

Discover ERBAqua®, Reagents for Karl Fischer titration

- For volumetric and coulometric titration
- Reliable reactivity
- Fast reaction
- Pyridine free
- Accurate and reproducible results
- Easy to use
- Wide range of solvents for the solubilization of the samples



Your partner in choice for Chemicals











www.carloerbareagents.com



serviciocliente@cer.dgroup.it

Tel: +34 93 693 37 35





export@cer.dgroup.it

Ph.: +33 2 32 09 20 00







CARLO ERBA Reagents S.r.I. Via Raffaele Merendi 22 20007 Cornaredo (MI)

Servizio Clienti

servizioclienticer@dgroup.it

Informazioni tecniche

chemicals@cer.dgroup.it Tel.: +39 02 93 99 190 Fax: +39 02 93 99 10 01



FRANCE

CARLO ERBA Reagents SAS Chaussée du Vexin, Parc d'affaire des Portes 27106 Val de Reuil

Service Client

serviceclient@cer.dgroup.it Tél.: +33 2 32 09 20 00 Fax: +33 2 32 59 11 89

DEUTSCHLAND

CARLO ERBA Reagents GmbH Denzlinger Str. 27 79312 Emmendingen

Kundendienst info.de@cer.dgroup.it Tel.: +49 07641 46 881 90 Fax: +49 07641 46 881 919

ESPAÑA

CARLO ERBA Reagents S.A. Calle Filadors 35, 6ª Planta Puerta 5 08208 Sabadell (BCN)

Servicio Cliente

serviciocliente@cer.dgroup.it Tel.: +34 93 693 37 35 Fax: +34 93 724 31 68

ALL OTHER COUNTRIES

Customer Service export@cer.dgroup.it Ph.: +33 2 32 09 20 00 Fax: +33 2 32 59 11 89









www.carloerbareagents.com